

Quantifying alterations over time in ST-segment/T-wave amplitudes during elective percutaneous coronary intervention

Philip Hempel, Theresa Bender, Ennio Idrobo-Ávila, Henning Dathe, Dagmar Krefting, Tim Kacprowski, Nicolai Spicher

Angaben zur Veröffentlichung / Publication details:

Hempel, Philip, Theresa Bender, Ennio Idrobo-Ávila, Henning Dathe, Dagmar Krefting, Tim Kacprowski, and Nicolai Spicher. 2023. "Quantifying alterations over time in ST-segment/T-wave amplitudes during elective percutaneous coronary intervention." *Computing in Cardiology Conference (CinC)* 50: ID 112.
<https://doi.org/10.22489/cinc.2023.112>.

Nutzungsbedingungen / Terms of use:

CC BY 4.0

Quantifying Alterations over Time in ST-segment/T-wave Amplitudes During Elective Percutaneous Coronary Intervention

Philip Hempel^{1,2}, Theresa Bender^{1,2}, Ennio Idrobo-Avila¹, Henning Dathe¹, Dagmar Krefting^{1,2},
Tim Kacprowski^{3,4}, Nicolai Spicher^{1,2}

¹ Department of Medical Informatics, University Medical Center Göttingen

² DZHK (German Centre for Cardiovascular Research), Partner Site Göttingen

³ Division Data Science in Biomedicine, PLRI of TU Braunschweig and Hannover Medical School

⁴ Braunschweig Integrated Centre of Systems Biology (BRICS), TU Braunschweig

Abstract

In this work, we evaluate the inter-patient magnitude of electrocardiography (ECG) alterations over time during ischemia. The freely available STAFF III database provides 12-lead ECG recordings of patients before, during, and after elective percutaneous coronary intervention (PCI), where a coronary vessel is widened with a balloon inflation. Patients undergoing this procedure often do not show standard ECG findings and thereby cannot be assessed by the subject-independent and absolute thresholds defined in clinical guidelines. We compute alterations of ST-segment and T-wave amplitudes w.r.t. QRS amplitude over time for each patient and lead. We demonstrate that quantifying these relative amplitudes changes over time is feasible in standard and non-standard ECG recordings. To demonstrate clinical relevance, we use the features for differentiating N=54 patients with atherosclerotic plaque in either the right coronary artery (RCA) or left anterior descending (LAD). Results show significant differences in five leads for ST-segment alterations and three leads for T-wave alterations, which are also suggested by clinical guidelines for ischemia detection.

1. Introduction

In elective PCI the chronically narrowed coronary arteries are opened to enable sufficient oxygen supply of the heart itself and improve quality of life for patients suffering from coronary artery diseases (CAD). In this non-surgical technique a catheter is inserted into an artery and advanced to the heart. After the exact location of the narrowed coronary vessel is determined, a balloon is inflated to widen the artery. In early days of PCI, the focus was on prolonged balloon inflation time in order to compress the atherosclerotic plaque with high pressure against the arterial wall, resulting in improved blood flow [1].

ECGs recorded during this – nowadays outdated – technique imitate the ECG alterations resulting from blocked coronary vessels, since there is strongly reduced blood flow in the vessel during balloon inflation. In the last decades, brief inflations with lower pressure and the usage of metal or plastic stents have been established to further reduce risk of life threatening complications [2]. Patients undergoing elective PCI have pre-existing heart conditions and often show non-standard ECG recordings, e.g. permanently altered amplitudes of the ST-segment and T-wave, which are hard to interpret using clinical guidelines [3,4]. Analyzing relative ST-segment/T-wave amplitudes over longer time – instead of absolute mV values extracted from 10-second ECGs as suggested in guidelines – could offer a novel view on non-standard ECGs.

Hence, in this work we work towards this aim by analyzing changes over time in the ST-segment and T-wave of patients undergoing PCI in either the RCA or LAD and use this information to differentiate both groups. The first supplies the posterior right side of the heart while the latter supplies the left anterior side of the heart and often shows laterally reversed ECG findings. We use the ST-segment amplitude as the slowed electric impulse, pointing in the direction of the ischemic region, can be detected on the affected site as ST-elevation and on the non-affected side as ST-depression [5].

2. Methods

We aim for quantifying ECG alterations over time in ischemic conditions. Thereby, we selected data of patients undergoing PCI and focus on the amplitude of the ST-segment, where regularly no electric activity of the heart can be measured in physiologic ECG recordings, and the amplitude of the T-wave, representing the repolarization of the ventricles. Both features are based on clinical guidelines for diagnosis of ischemia with the amplitude of the

ST-segment being an established parameter [5–7].

Dataset The STAFF III database contains 12-lead ECGs from 104 patients treated with the outdated technique of elective prolonged balloon inflation in a major coronary artery [8]. The ECGs were acquired from 1995 to 1996 at Charleston Area Medical Center (WV, USA) and sampled at 1000 Hz with an amplitude resolution of $0.6 \mu\text{V}$. Custom-made equipment by Siemens-Elema AB (Sweden) was used to record standard chest leads and limb leads in the Mason-Likar configuration.

The pre- and post-inflation ECGs were both recorded 5 min in supine position at rest, in a baseline room before and lying in the catheter lab after PCI. The mean inflation time was 4 min 23 s, ranging from 1 min 30 s to 9 min 54 s with exact annotations provided, including time and localization of the balloon inflation [8].

All patients that underwent primary balloon inflation in the RCA or LAD were processed. We analyze 23 patients (age: 60 ± 12 years; 48% female) with balloon inflation in the LAD and 31 patients (age: 58 ± 8 years; 42% female) with balloon inflation in the RCA. For each patient, several ECGs were measured at three different stages: i) pre-inflation, ii) during-inflation and iii) post-inflation.

Preprocessing In order to reduce noise, a single representative beat [9] is calculated using the function `ecg_segment` of the open-source library Neurokit2 [10]. For this computation, single heart beats are temporally aligned using the R-peaks detected by Kalidas algorithm [11]. Additionally, the quality of these heart beats is calculated using the function `ecg_quality` of Neurokit2 [10] and only heart beats with at least 80% similarity to the others are included. After selecting the lead with the highest R-peak amplitude, the ECG signal is delineated using the function `ecg_peaks` of Neurokit2 [10]. The T-, P- and R-peaks of this lead are then transferred to all other leads and their positions are corrected within a range of 40 ms to address minimal deviations between leads.

Feature engineering We define the ST-segment as a 40 ms segment starting 85 ms after the R-peak according to García *et al.* [6]. The isoelectric line is defined as the mean amplitude of the TP-interval, calculated within physiologic boundaries of 50 ms after the T-peak and 40 ms before the P-peak. This enables to evaluate the amplitudes of the ST-segment and the T-peak in relation to QRS-amplitude, which we will denote "ST feature" and "T feature", respectively. According to Aslanger *et al.*, this approach based on relative differences has the advantage of including the cardiac vector information in contrast to absolute quantification in mV [5].

For each patient and lead, features are computed in overlapping intervals of 50 s with steps of 10 s. In order to quantify the dynamic of the features measured during

stages pre-inflation (i) and during-inflation (ii), the difference between average values of both stages is computed (ii-i), which we will denote " ΔST " and " ΔT ".

Statistical analysis In order to evaluate the differences in alterations over time between LAD and RCA patients, we test for statistical differences. First, the null hypothesis whether the groups are normally distributed is tested in every lead using a Jarque–Bera test. Second, the null hypothesis is tested that the variances of both groups do not differ for every lead and feature using a two-sided t-test.

3. Results

Fig. 1 shows representative beats (panel 1,3) and the alterations over time (panels 2,4) for an RCA and LAD patient, respectively. Lead V2 shows alterations over time for ST mainly within the balloon inflation time. During occlusion of RCA, this results in a constant decrease of ST and T features, visible in the representative beat (panel 1) and the calculated relative values (panel 2). In contrast, an occlusion of LAD results in a constant increase of ST and T within the representative beat (panel 3) and relative values (panel 4). The LAD patient shows a non-standard ECG, presumably due to a pre-damaged heart, which is expressed by ST-elevation before balloon inflation. Regarding the T feature, alterations over time (panels 2, 4) show a similar behavior in the during-inflation stage.

Fig. 2 summarizes ΔST and ΔT features representing the differences between the stages pre-inflation and during-inflation in every lead and patient. For ΔST , leads V2-V4 show higher values for LAD patients compared to RCA patients. In leads II-III the results are reversed with RCA patients showing higher values. Regarding ΔT , in leads V2-V4 the same effect as in ΔST can be seen, while leads II-III do not show clearly effects. The differences in leads V2-V3 and II-III are highly significant for ΔST , whereas in ΔT only V2-V3 are highly significant.

4. Discussion

This work was motivated by the assumption that changes in relative ST-segment/T-wave amplitudes over time could be a useful feature in non-standard ECGs.

The proposed dynamic for ischemic ECG alterations over time in patients undergoing prolonged balloon inflation show a potential for differentiating LAD and RCA patients. The features in the LAD patients are very similar to clinical findings, where standard ECGs show characteristic ST-elevation in leads V2-V4 with contralateral ST-depressions in leads II and III [5]. *Vice versa*, laterally-reversed ECG findings can be found in RCA patients using our features which is also covered by clinical guidelines [5].

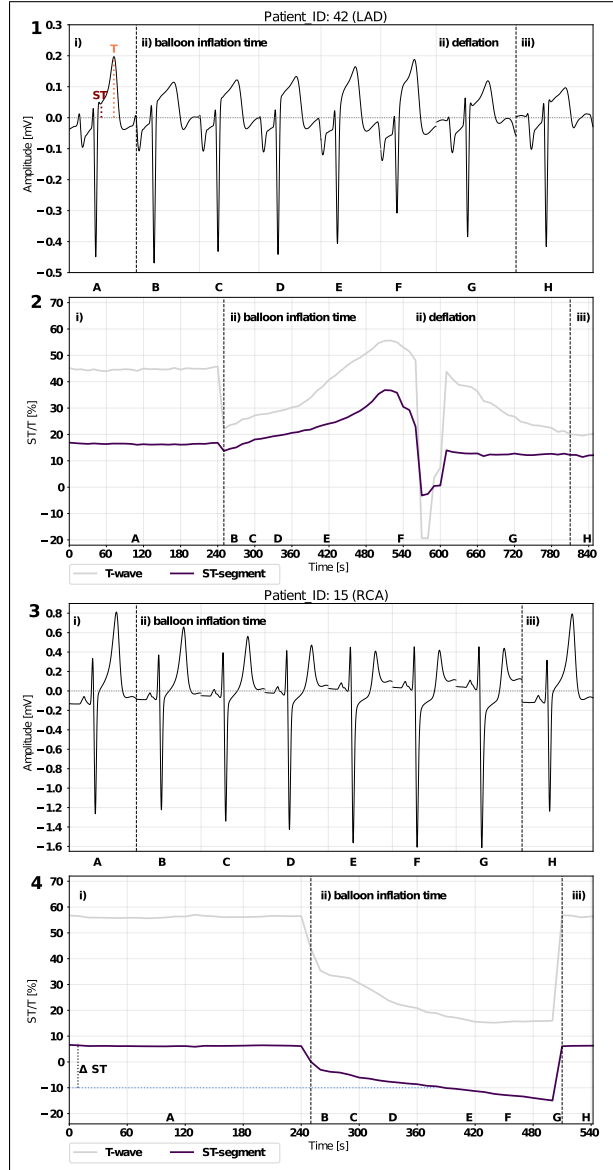


Figure 1: Lead V2 features during elective PCI for an RCA patient (panels 1-2) and LAD patient (3-4). Representative beats (1,3) and ST and T feature (2,4) computed over time during three stages are shown: i) pre-inflation ii) during-inflation iii) post-inflation. In the LAD patient, stage ii) additionally shows the moment of balloon deflation within the recording. Vertical, dashed lines mark interruptions in measurements due to medical intervention. A-H show occurrences in time of the representative beats and their value w.r.t. QRS amplitude. In panel 1, the ST and T feature of the first representative beat are shown. In panel 4 bottom left, the computation of the alterations over time ΔST are depicted exemplary.

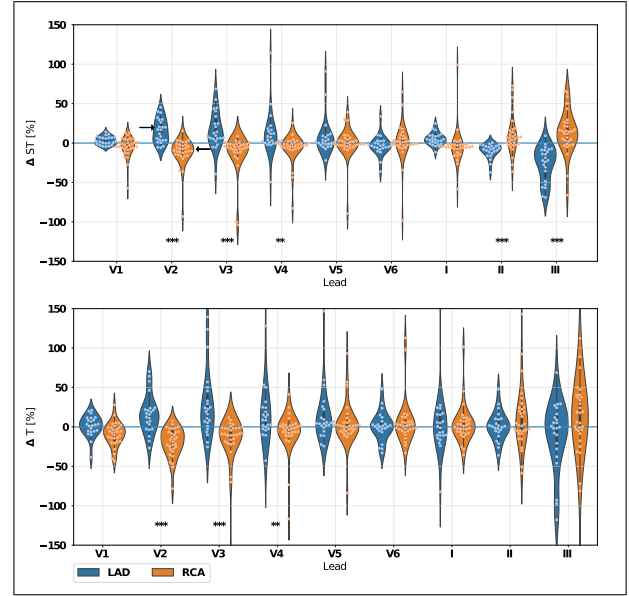


Figure 2: ΔST and ΔT features of LAD (blue) and RCA (orange) patients. Each point corresponds to a patient. In leads V2-V4 both groups can be easily distinguished from each other. The black arrows indicate the data points for patients 42 and 15 in ΔST . *** indicates a significance with $p \leq 0.001$ and ** indicates $0.001 < p \leq 0.01$.

However, clinical guidelines use 10-second 12-lead ECGs representing only a snapshot of the current cardiac activity and look for absolute alterations in mV. We demonstrate that it is also feasible to detect alterations over time based on relative values as proposed by cardiologists [8] and researchers [5]. In Fig. 1 the pre-inflation ECG of LAD patient 42 already shows an elevated ST-segment amplitude. This ST-elevation is problematic as the conventional assessment prevents proper diagnosis of life-threatening restenosis. However, our proposed dynamic w.r.t. ΔST and ΔT show characteristic changes over time, which could be an avenue for future work for more accurate diagnosis.

In the recent guideline for evaluation of chest pain, the T-wave is not taken into account considerably. However, there are many researchers trying to improve diagnosis based on T-wave features [7]. Within the STAFF III database, García et al. [6] found that in 72% of patients with ST-segment amplitude changes were also showing T-wave amplitude changes. Martínez et al. [12] studied the prevalence, magnitude and spatio-temporal relationship between T-wave alternans and ischemia. They analyzed the ECGs beat by beat and found T-wave alterations in 33.7% of the patients. A reason why usage of T-waves is challenging can be seen in the pre-inflation ECG of patient 42 (panel 1) in Fig. 1: The T-wave (A) shows a similar

height as during balloon inflation (F), highlighting its morphological variability. A potential explanation could be that the ECG was detached and re-attached between both stages. Our results also indicate that the T-wave might be a useful additional feature for monitoring of ischemic ECG alterations if the device is constantly attached.

A limitation of this work is that we only analyzed a single database. Therefore, investigating whether the observed alterations can also be noticed in other patient cohorts and is not present in healthy subjects is an avenue for future work. Additionally, we plan to extend the investigation on other coronary vessels like left circumflexum (LCx) since this type of ischemia is often underdiagnosed. In these ECGs, anterior ST-depression dynamics could potentially point towards posterior ST-elevation which could be checked by using additional leads V7-V9 [8].

5. Conclusions

In this work, two established ECG features, namely the amplitudes of the ST-segment and T-wave [2, 13], were extended by quantifying them i) over time and ii) as relative values w.r.t. QRS complex amplitude. Using these novel features, we found significant differences between LAD and RCA patients when comparing ECGs before and during PCI. This approach extends the state-of-the-art based on subject-independent and absolute thresholds defined in clinical guidelines. The dynamic of the features could be useful for patients in which these “one size fits all” thresholds fail, e.g. in patients showing only subtle alterations [14] or with permanent ST-alterations [15]. However, further studies with different patient cohorts and larger datasets in general are required to investigate whether the proposed dynamic could further improve the detection of cardiac ischemia using standard 12-lead ECGs.

References

- [1] Moorman DL, Kruger WB, Jackson WG. Percutaneous transluminal coronary angioplasty (PTCA): long-term outcome and aeromedical implications. *Aviation Space and Environmental Medicine* October 1996;67(10):990–996. ISSN 0095-6562.
- [2] Katz G, Harchandani B, Shah B. Drug-Eluting Stents: the Past, Present, and Future. *Current Atherosclerosis Reports* March 2015;17(3):11. ISSN 1523-3804, 1534-6242.
- [3] Di Toro M, Stub D. Acute Myocardial Infarction Identified by Paramedics Using the Smith-Modified Sgarbossa Criteria: A Case Report. *Prehospital Emergency Care* November 2021;25(6):851–853. ISSN 1090-3127, 1545-0066.
- [4] Bhatt DL, Lopes RD, Harrington RA. Diagnosis and Treatment of Acute Coronary Syndromes: A Review. *JAMA* February 2022;327(7):662. ISSN 0098-7484.
- [5] Aslanger, Emre K. and Meyers, H. Pendell and Smith, Stephen W. Recognizing electrocardiographically subtle occlusion myocardial infarction and differentiating it from mimics: Ten steps to or away from cath lab. *Türk Kardiyoloji Dernegi Arsivi Archives of the Turkish Society of Cardiology* September 2021;49(6):488–500.
- [6] García J, Lander P, Sörnmo L, Olmos S, Wagner G, Laguna P. Comparative Study of Local and Karhunen–Loève-Based ST–T Indexes in Recordings from Human Subjects with Induced Myocardial Ischemia. *Computers and Biomedical Research* August 1998;31(4):271–292. ISSN 00104809.
- [7] Demidova MM, Martín-Yebra A, Martínez JP, Monasterio V, Koul S, van der Pals J, Romero D, Laguna P, Erlinge D, Platonov PG. T wave alternans in experimental myocardial infarction: Time course and predictive value for the assessment of myocardial damage. *Journal of Electrocardiology* May 2013;46(3):263–269. ISSN 00220736.
- [8] Laguna P, Sörnmo L. The STAFF III ECG database and its significance for methodological development and evaluation. *Journal of Electrocardiology* July 2014;47(4):408–417. ISSN 00220736.
- [9] DiPietroPaolo D, Müller HP, Erné SN. A novel approach for the averaging of magnetocardiographically recorded heart beats. *Physics in Medicine and Biology* May 2005;50(10):2415–2426. ISSN 0031-9155, 1361-6560.
- [10] Makowski D, Pham T, Lau ZJ, Brammer JC, Lespinasse F, Pham H, Schölzel C, Chen SHA. NeuroKit2: A Python toolbox for neurophysiological signal processing. *Behavior Research Methods* August 2021;53(4):1689–1696. ISSN 1554-3528.
- [11] Kalidas V, Tamil L. Real-time QRS detector using Stationary Wavelet Transform for Automated ECG Analysis. In 2017 IEEE 17th International Conference on Bioinformatics and Bioengineering (BIBE). Washington, DC: IEEE. ISBN 978-1-5386-1324-5, October 2017; 457–461.
- [12] Martinez J, Olmos S, Wagner G, Laguna P. Characterization of Repolarization Alternans During Ischemia: Time-Course and Spatial Analysis. *IEEE Transactions on Biomedical Engineering* April 2006;53(4):701–711. ISSN 0018-9294.
- [13] Al-Alusi MA, Ding E, McManus DD, Lubitz SA. Wearing Your Heart on Your Sleeve: the Future of Cardiac Rhythm Monitoring. *Current Cardiology Reports* December 2019;21(12):158. ISSN 1523-3782, 1534-3170.
- [14] Jansen van Rensburg R, Schutte J, De Beenhouwer T. Chest pain: the importance of serial ECGs. *Journal of Medicine* 2021;88(10):538–540.
- [15] Manne JRR. Atrial repolarization waves (Ta) mimicking inferior wall ST segment elevation myocardial infarction in a patient with ectopic atrial rhythm. *Case Reports in Medicine* 2018;2018(1015730).

Address for correspondence:

Philip Hempel

Department of Medical Informatics, University Medical Center
Göttingen, 37075 Göttingen, Germany

philip.gemke@med.uni-goettingen.de